



भारतीय मानक ब्यूरो
BUREAU OF INDIAN STANDARDS
Mumbai Branch Office - II

Address Manakalaya, F9 MIDC, Andheri East
: Mumbai-400093
Phones :022-28329295, 28327892
Fax: 022-28264352
E-Mail: mubo2@bis.gov.in
web : <http://www.bis.org.in>

REGISTERED A/D

Our Ref :CM/L-7800023011

Dated :18
Apr 2017

Subject: Grant of BIS Certification Marks Licence No. CM/L-7800023011 as per IS 15351 : 2015

GULNAR PLASTICS PVT LTD,
SURVEY NO.18/P KHADARPADA ROAD, SILVASSA,
SILVASSA
Distt : Dadra and Nagar Haveli
396230

Dear Sir,

With reference to your application, we are pleased to inform you that it has been decided to grant you a licence to use the Standard Mark in respect of the following:

Product: Agro Textiles - Laminated High Density Polyethylene (HDPE) Woven Geomembrane for waterproof lining.

IS No : IS 15351 : 2015

Type/Size/Grade/Variety covered under licence :

Laminated HDPE woven Geomembrane for Waterproof lining, Type II" as per IS 15351:2015

2. The licence is being granted with the explicit condition that you will mark entire/substantial production which conforms to the Indian Standards referred above.

3.The number assigned to this licence is CM/L- 7800023011 which has been made operative from 17/04/2017 and is valid up to 16/04/2018. The licence number should invariably be referred to in your future correspondence.

4.According to sub-regulation (2) of Regulation 6 of Bureau of Indian Standards (Certification) Regulation, 1988, the licence fee of Rs 1000/- and the marking fee of Rs. 47300.00as stipulated in the Second Schedule of this licence is payable by you with effect from 17/04/2017 for the period of validity of the licence.

Service tax @ 15 % as applicable shall also be charged.

5. Minimum marking fee stipulated therein is payable by you regardless of the whether you actually mark your product or not with the Standard Mark. Our Receipt No. 7815271 dated 18/04/2017 for Rs. 63595.00 for the licence fee (Rs.1000/-) and the minimum marking enclosed/sent separately.

6. This advance minimum marking fee will be carried over to the next year on every renewal. The actual marking fee calculated on the unit rate on the production marked or the minimum marking fee, whichever is higher shall be payable by you at the time of renewal.

7. With a view to streamlining the reporting of quantity marked, calculation and collections of marking fee on the unit rate basis, fees will be calculated on the production marked during the first nine months of operation of the licence at the time of first renewal and the production marked during twelve months comprising the last three months of the previous operative year, at the time of second and subsequent renewals. In case the licence expires, the entire production marked till the expiry date shall be taken into account for calculating the marking fee payable.

8. The Scheme of Testing and Inspection DOC: STI/15351/2:SEPT 08 AMD-1 which has already been accepted by you vide your letter dated will have to be implemented by your organization strictly and control function in your organization. The supervision of the operation of the Scheme shall be done by a person responsible for the quality control function in your organization. Kindly inform us the name and designation of the person who will be held responsible for the operation and maintenance of the Scheme. Any future change in this respect will have to be communicated by you to us and whenever this takes place.

9. We are enclosing a sheet giving the preferred dimensions of the Standard Mark to enable you to prepare the designs of the Standard Mark for marking the above product. Photographic reduction in any size is permissible. This will ensure the relative proportions of the different dimensions are maintained. Preferred dimensions may be used as far as possible. Kindly get the designs of the stencil/label/rating plate incorporating the Standard Mark approved by us. You will be permitted to commence marking the above mentioned product only after approval by this office.

10. On commencement of marking of your product for which you are licensed, you may advertise your product with Standard Mark in hoardings, slides and newspapers only during the validity of your licence. The use of Standard Mark on letterheads and publicity literature will be permitted only on receipt of your assurance that in the event of cancellation or lapsing of your licence, the letterheads etc. with the Standard Mark will be destroyed/obliterated. The required assurance may please be submitted in the enclosed proforma.

11. You are requested to intimate us the actual date from which you intend to introduce the use of Standard Mark on your product. Our Inspecting Officer may be present in your factory at that time to assist you in adopting the Scheme of Testing and Inspection (STI) and in the maintenance of test records.

12. The Licence is being granted for you factory situated at : SURVEY NO.18/P KHADARPADA ROAD, SILVASSA SILVASSA Dadra and Nagar Haveli and the rights and privileges under the licence shall not be exercised by any other firm/company/factory, etc. This licence is not transferable. In the event of shifting of the manufacturing and testing equipment from the licenced premises to some other place, use of Standard Mark shall be stopped till the new premises are inspected and found to be satisfactory by us in respect of manufacturing and testing facilities available there and address of the new premises is endorsed in the licence.

13. A copy/copies of test report(s) of the sample(s) drawn at the time of preliminary inspection of your factory is/are enclosed for your records.

14. You are requested to intimate to this office the address of your servicing unit where applicable and the name and designation of the person, his telephone and telex number who should be contacted in case of complaints. It is obligatory on your part as a licensee to keep this office informed about changes taking place from time to time in your declared list of servicing units.


15. The licence is under preparation and will be posted to you in due course.

16. You are requested to send us back the enclosed proforma No. CMD/PF615 duly filled in.

17. An instruction sheet containing Responsibilities of BIS Licensees is also enclosed for information / compliance.

Kindly acknowledge receipt of this letter.

Thanking you,



(Rajeev P)
Scientist 'E' & Head

to the standard mark indicated in your member magazine and note that:

- a) Photographic reduction in any size of Figure 1 is permissible; and
- b) Preferred dimensions as given in Table 1 be used as far as possible.

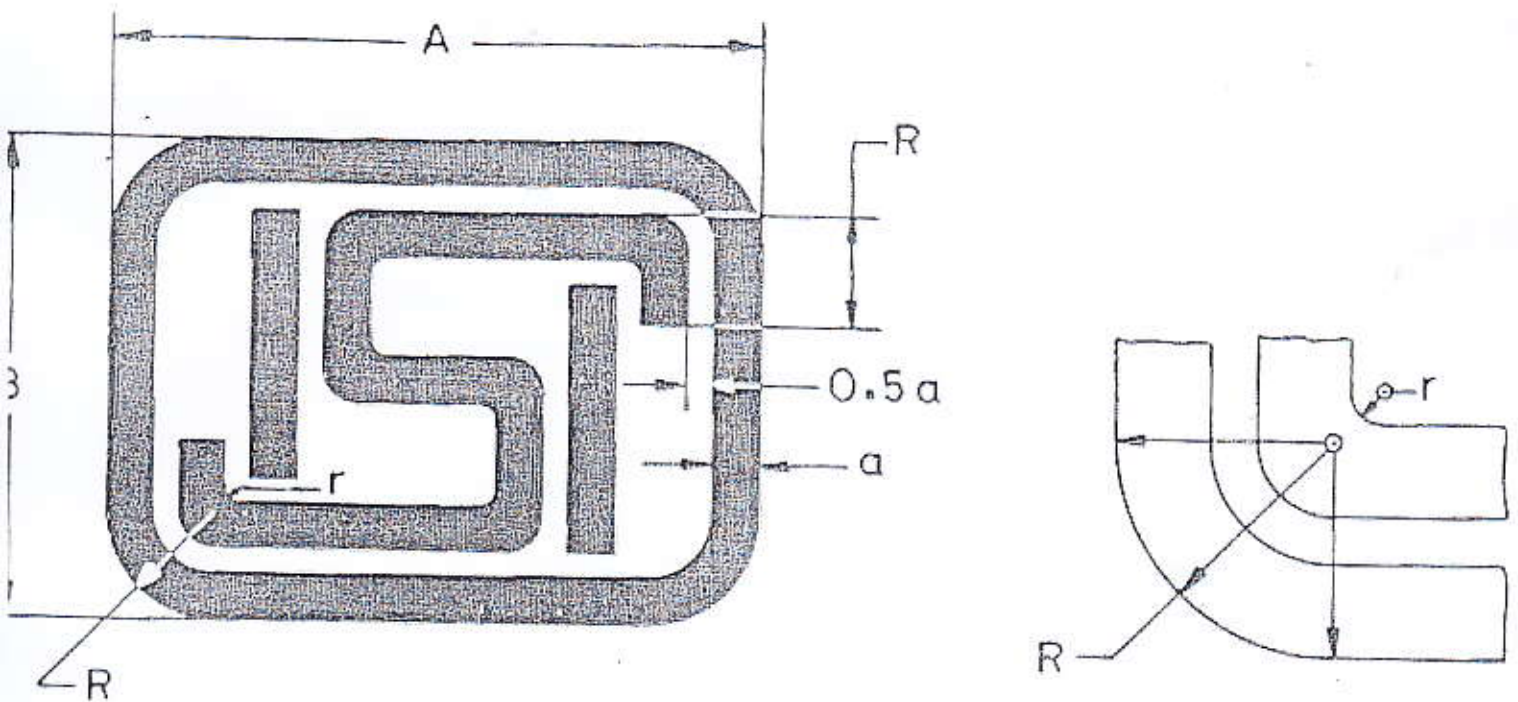


FIG. 1

TABLE 1 PREFERRED DIMENSIONS OF ISI MONOGRAM
All dimensions in millimetres

A	B	a	R	r	SIZE OF LETTERS
2.5	1.9	0.2	0.4	-	1.0 mm
5	3.8	0.4	0.8	0.1	1.0 mm
10	7.5	0.7	1.7	0.2	2.0 mm
20	15	1.5	3.3	0.5	3.0 mm
40	30	2.9	6.7	1.0	4.0 mm
80	60	5.9	13.4	1.9	6.0 mm
160	120	11.7	26.7	3.8	10.0 mm
320	240	23.4	53.4	7.6	16.0 mm